

# nelis

GLOVE PORT

This is the real single port.



# Glove port **A version**

Glove port A version can be open during operation. It's easy to extract with surgical specimen during operation



## ● Flexibility

Glove port provides the surgeons free of motion when they perform the surgery.




## ● Can be used in Robotic surgery



## ● Clear port head

Glove port has crystal clear port head. It helps doctors prevent instruments fight by watching them intuitively.



## ● Various models

Glove port has models for robotic surgery can be performed with Da Vinci, and Transvaginal surgery also.



## ● Detachable design



## ● Easy docking


Glove port needs simple procedure docking before surgery.



# Glove port in **Robotic surgery**




## ● Characteristics of Glove port in Robotic Surgery

1. Transparent Head to prevent instrument fight
2. Easy to identify internal bleeding
3. Easy to make fine movement by flexible
4. A number of models make the surgery easy to apply the various instrument
5. Elasticity of Cook Cap is easy to insert

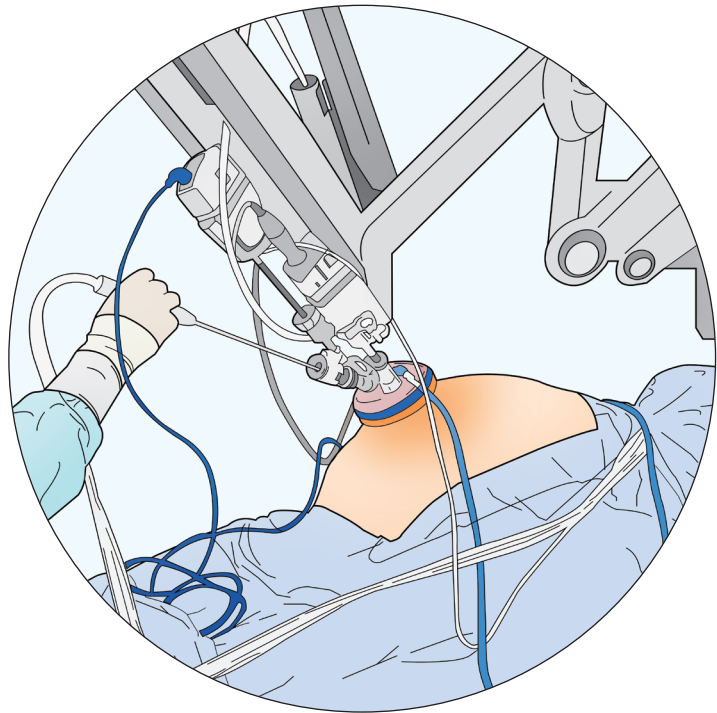

## ● Characteristics of Glove port in Robotic breast Surgery

1. Minimize surgical scars
2. Expanded Surgical View
3. If total ablation is needed, simultaneous breast reconstruction is possible

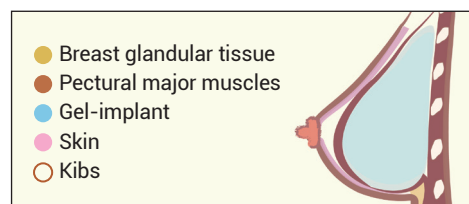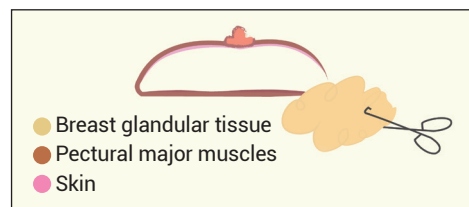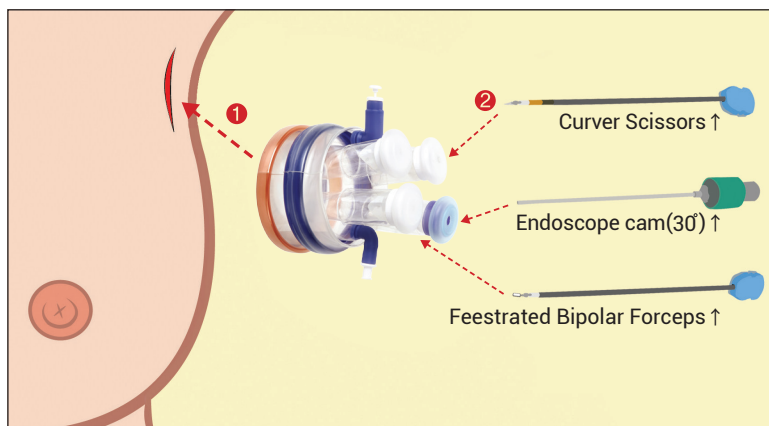

\* ROBOTIC NIPPLE-SPARING MASTECTOMY AND IMMEDIATE BREAST RECONSTRUCTION WITH GEL IMPLANT :  
TECHNIQUE, PRELIMINARY RESULTS AND PATIENT-REPORTED COSMETIC OUTCOME, Hung-Wen Lai, MD, PhD, Shou-Tung Chen, MD, Shih-Lung Lin, MD, Chih-Jung Chen, MD, PhD, Ya-Ling Lin, BS, Shu-Hsin Pai, BS, Dar-Ren Chen, MD, (2018), 2 page.



GLOVE PORT 4-Head



GLOVE PORT 5-Head



GLOVE PORT 6-Head

## | Applicable operation

Operation	A version	Original	P version
Appendectomy	431AS, 431AM	440, 431	
Gall Bladder			
Cholecystectomy			
Urinary Tract Stone Removal			P431
Urology			
Uterine Myoma	431AS, 330AS	330, 431	
Ovariectomy			
Endometriosis			P321
Colorectal surgery	422AS, 431AM	422	
Hysterectomy			
Hysteromyomectomy with morcellator	422AS-15, 422AM-15		P422-15
Gastrectomy	422AM, 431AM		
Paediatric surgery	431AT, 440AT, 4220AT		
Robot surgery	642-AL-1-1, 541AM-2W		

\* Ectopic pregnancy, Fibroids, Hepatectomy and so on.

\* The size of the port (S,M,L) depends on proficiency, incision size, and the size of the incised tissue.

**NELIS**

**NELIS CO., LTD**  
 1005, 201-dong, 397, Seokcheon-ro, Bucheon-si, Gyeong-gi-do, 14449, Korea  
**Tel :** + 82 32 624 1697 **Tax :** + 82 32 624 1699  
**Email :** nelismed@daum.net / nelismedical@naver.com  
**Website :** nelis.co.kr

**MEDITECH**  
**INFRAMED**

**MEDITECH-INFRAMED CO., LTD**  
 515, Dongnam-ro, Gangdong-gu, Seoul, Republic of Korea  
**Tel :** + 82 2 476 8381 **Fax :** + 82 2 476 1640  
**Email :** inframed@empas.com  
**website :** inframed.co.kr